



PrymaLab

PRYMALAB ANALYTICAL · IN-HOUSE LABORATORY

3705 Music Branch Rd, Ashland, KY 41102 · +1 (606) 465-9063 · prymalab.net



CERTIFICATE NO.
PL-26-00028

VERIFICATION KEY
UTXGB3N9

Scan or enter both at
prymalab.net/testing/verify

CERTIFICATE OF ANALYSIS · LOT RELEASE

DSIP 10 mg

Lot PL-2609-028 · Lyophilized powder · Label claim 10 mg/vial

TESTED IN-HOUSE BY PRYMALAB

In-house analytical result,
not an independent third-party test

LOT / BATCH NUMBER PL-2609-028	DATE MADE 2026-09-17	DATE OF ANALYSIS 2026-09-18	DATE ISSUED 2026-10-03
RETEST / EXPIRY 2028-09-17	UNITS IN LOT / SAMPLED 250 / 2	STORAGE -20 °C, desiccated, dark	CERTIFICATE TYPE Lot COA, 2 pages
COMPOUND DSIP Delta sleep-inducing peptide	CAS NUMBER 62568-57-4	MOLECULAR FORMULA $C_{35}H_{48}N_{10}O_{15}$	THEORETICAL MASS (AVG.) 848.8 Da
SEQUENCE H-WAGGDASGE-OH (9 residues; free N- and C-termini)			

PURITY · RP-HPLC, AREA %

99.52%

Specification 99.0% • main peak at 4.78 min

IDENTITY · OBSERVED MASS

849.0 Da

Theoretical 848.8 Da • +0.2 Da (236 ppm)

OVERALL CONCLUSION


PASS

Meets every specification for the tests performed

TEST	METHOD	SPECIFICATION	RESULT	CONCLUSION
Appearance	Visual inspection	White to off-white lyophilized powder	White lyophilized powder	PASS
Identity (mass)	LC-MS, ESI positive	Theoretical $\pm$ 1.0 Da	849.0 Da	PASS
Purity	RP-HPLC, UV 214 nm, area%	99.0%	99.52%	PASS
Largest impurity	RP-HPLC, area%	1.0%	0.18% at 5.62 min	PASS
Water content	Karl Fischer	5.0%	1.7%	PASS
Bacterial endotoxin	LAL, kinetic	$\leq$ 5.0 EU/mg	0.03 EU/mg	PASS
Sterility / bioburden	USP <71>, membrane filtration	No growth after 14 days	No growth; conforms	PASS

1 HPLC CHROMATOGRAM

Data file: DSP_PL-2609-028_20260918_01 · Column C18 150 $\times$ 4.6 mm · UV 214 nm

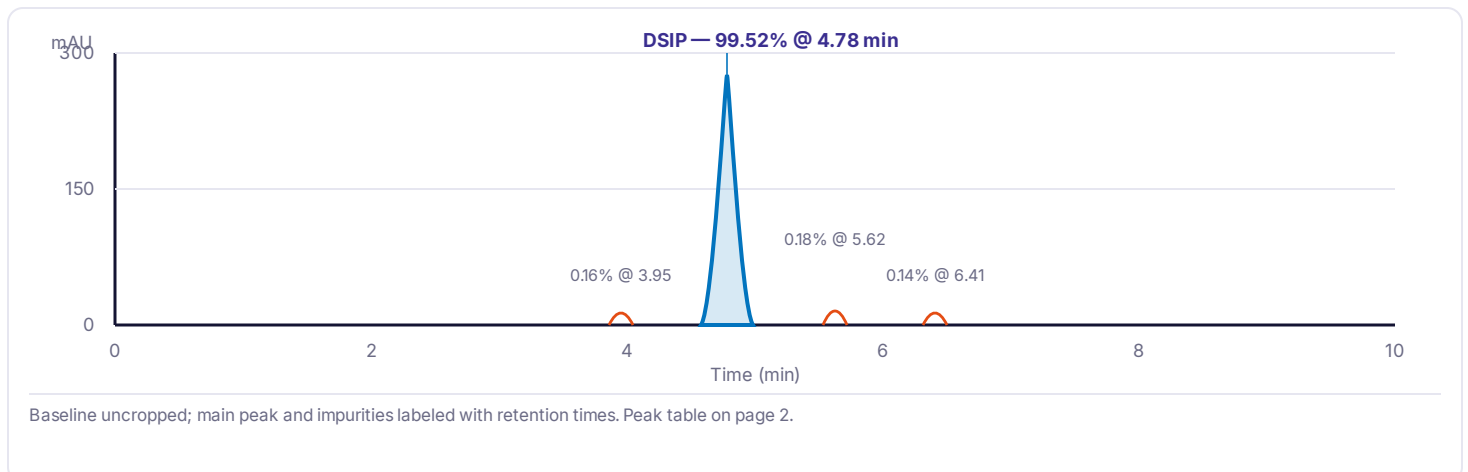

**2 HPLC METHOD · DSP_PL-2609-028_20260918_01**

INSTRUMENT

Waters Alliance e2695, SN E2695B742

DETECTION WAVELENGTH

214 nm

MOBILE PHASE A

0.1% TFA in water

COLUMN TEMPERATURE

30 °C

SAMPLE DILUENT

Water, 0.1% TFA

REFERENCE STANDARD

In-house DSIP reference, lot PL-RS-DSP-01, RT 4.76 min

DATA SYSTEM

Empower 3, Build 3471

COLUMN

C18, 150 × 4.6 mm, 3.5 µm

MOBILE PHASE B

0.1% TFA in MeCN

INJECTION VOLUME

20 µL

SAMPLE CONCENTRATION

0.5 mg/mL

DETECTOR

Waters 2998 PDA

COLUMN PART / SERIAL

186003326 / USHX18211

FLOW RATE

1.0 mL/min

RUN TIME

10 min

BLANK INJECTED

Yes

3 GRADIENT PROGRAM

TIME (MIN)	% A	% B
0.0	95	5
3.0	95	5
7.0	55	45
8.0	20	80
9.0	20	80
10.0	95	5

4 PEAK TABLE

PEAK	RT (MIN)	AREA	AREA %
1	3.95	6,800	0.16
2	4.78	4,229,600	99.52
3	5.62	7,650	0.18
4	6.41	5,950	0.14
Total		4,250,000	100.00

Threshold 0.05% area · Blank subtracted: Y · Purity = main peak area ÷ total integrated area × 100, to two decimals; main peak shaded.

5 IDENTITY BY MASS SPECTROMETRY

INSTRUMENT

Waters Acquity SQD

DECONVOLUTED MASS

849.0 Da

DATA FILE

DSP_PL-2609-028_MS_20260918_01

IONIZATION / MODE

ESI, positive

THEORETICAL MASS

848.8 Da

ACCEPTANCE

Within ± 1.0 Da

OBSERVED M/Z (CHARGE)

849.7 (1+ [M+H]) · 871.7 (1+ [M+Na])

DIFFERENCE

+0.2 Da (236 ppm)

6 ADDITIONAL TESTS

TEST	PERFORMED BY	DATE	REPORT / FILE
Water content	PrymaLab	2026-09-19	RPT-KF-PL-2609-028
Endotoxin	PrymaLab	2026-09-20	RPT-ET-PL-2609-028
Sterility	PrymaLab	2026-10-02	RPT-ST-PL-2609-028

A test with no row here was not performed on this lot. Outside-laboratory reports, when used, are attached and named below.

7 REVIEW AND APPROVAL**D. Reynolds**

Analyst · performed the testing

Date: 2026-09-18

S. Calloway

Reviewer · checked against raw data

Date: 2026-10-02

M. Phelps

Lab Director · approved for release

Date: 2026-10-03

Raw data retained at: Empower 3 (Build 3471), project PL-2609, archive PL-ARC-2026; 7 years. Outside laboratory reports attached: None

This certificate applies only to the lot named above and describes the units sampled from it; it is not a guarantee for any other lot. Results were obtained by PrymaLab LLC's own laboratory (PrymaLab Analytical) and are not an independent third-party test unless an outside report is attached. Reference values (CAS, formula, theoretical mass, sequence) are literature values for the named compound. Authenticity: scan the QR code or enter certificate number PL-26-00028 and key UTXGB3N9 at prymalab.net/testing/verify; any copy that does not match the record shown there is not a PrymaLab certificate. PrymaLab LLC products are supplied for laboratory research use only and not for human or veterinary use.